

# Vet X-Ray System Touch Screen

High-frequency X-ray System

## WARRIOR RT 400 HF/TS

generator 30 kW, 125 KV, power 3 kW

The radiographic equipment is composed from:

Generator, monoblock and high frequency Rack  
from 99-125 kV and 400 mA.

The radiographic system working can be:

### MANUAL

The operator chooses the parameters of kW and mAs as needed.

### ANATOMIC

The operator select the anatomic part.

The radiographic equipment is complete with grid.

**Operative mode 2-3 point selectionable by software.**

OPERATOR  
INTERFACE  
TOUCH SCREEN



### CONTROL PANEL

Power supply	230V 50Hz monofase
Power consumption	3 kW
Adjustment kV	from 40 kV to 99 or 125 kV
MAs adjustment	from 0.6 to 250 mAs
Adjustment ms	from 4 to 1000 ms

### Touch Screen Panel 7" TFT

### Software signal system state

**Dedicate memory area of password levels warning  
per service analysis**

### SAFETY DEVICE

- ✓ Device that allows the tube RX always work within the load curve.
- ✓ Visual indicator and audible presence of the x-ray radiography performed.
- ✓ Inverter protection.
- ✓ **Different level password for the system**

### MONOBLOCK

#### MODEL

Current max generator  
Max power generator  
Radiation leakage

#### RT 400 HF

400mA  
30kV  
less than 1 mGy/hour  
according to IEC 601-1-3



#### RX TUBE

Type  
Focus  
Maximum value

Rotating anode  
0,6 / 1,3 mm  
130 kV

### OPTIONAL

- ✓ Special RX length table, upon request, up to 2 m
- ✓ Signal lamp outside the presence of RX
- ✓ cable lenght control pedal

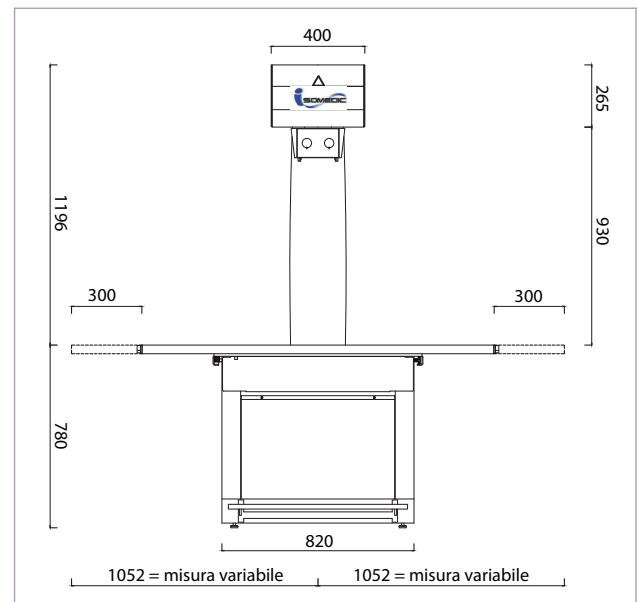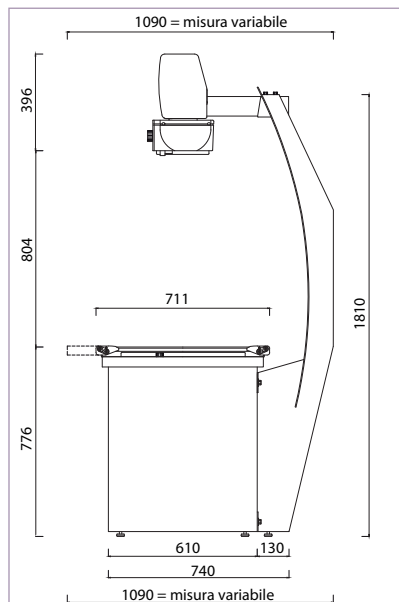

# Vet X-Ray System Touch Screen

High-frequency X-ray System

## WARRIOR RT 200 HF/TS

generator 15 kW, 125 KV, power 3 kW

The radiographic equipment is composed from:

Generator, monoblock and high frequency Rack from 99-125 kV and 200 mA.

The radiographic system working can be:

### MANUAL

The operator chooses the parameters of kW and mAs as needed.

### ANATOMIC

The operator select the anatomic part.

The radiographic equipment is complete with grid.

**Operative mode 2-3 point selectable by software.**

OPERATOR  
INTERFACE  
TOUCH SCREEN



### CONTROL PANEL

Power supply	230V 50Hz monofase
Power consumption	3 kW
Adjustment kV	from 40 kV to 99 or 125 kV in steps 1 kV
MAs adjustment	from 0.6 to 250 mAs
Adjustment ms	from 4 to 1000 ms

**Touch Screen Panel 7" TFT**

**Software signal system state**

**Dedicate memory area of password levels warning per service analysis**

### SAFETY DEVICE

- ✓ Device that allows the tube RX always work within the load curve.
- ✓ Visual indicator and audible presence of the x-ray radiography performed.
- ✓ Inverter protection.
- ✓ **Different level password for the system**

### MONOBLOCK

#### MODEL

Current max generator  
Max power generator  
Radiation leakage

#### RT 200 HF

200mA  
15kV  
less than 1 mGy/hour  
according to IEC 601-1-3



#### RX TUBE

Type  
Focus  
Maximum value

Rotating anode  
0,6 / 1,3 mm  
130 kV

### OPTIONAL

- ✓ Special RX length table, upon request, up to 2 m
- ✓ Signal lamp outside the presence of RX
- ✓ cable lenght control pedal

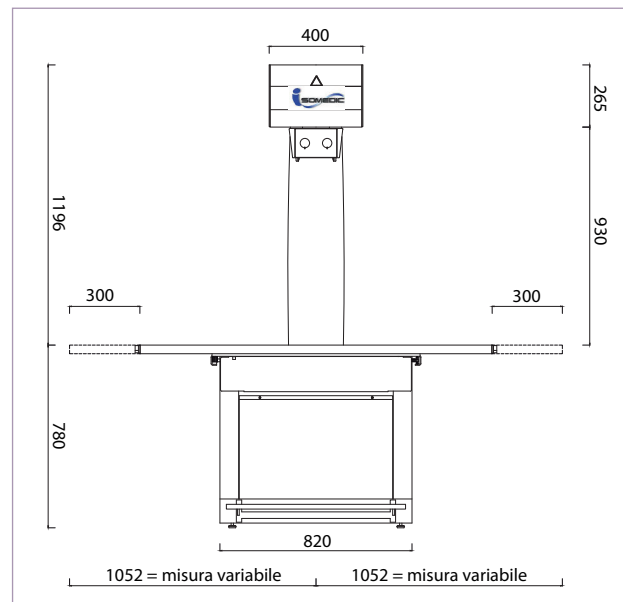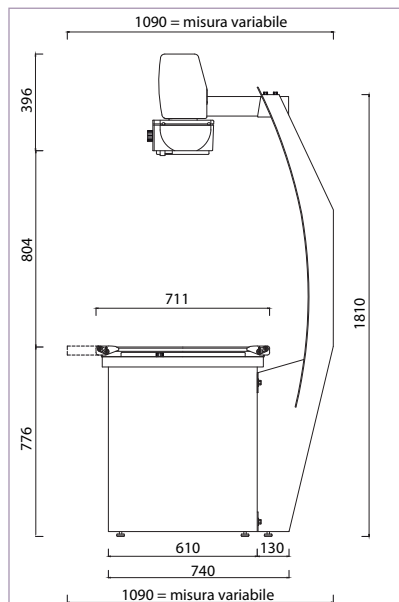

Aquarius Centre, Edison Close, Waterwells Business Park, Quedgeley, Gloucestershire, GL2 2FN

Tel: 01452 347101 Email: [info@photonsurgicalsystems.co.uk](mailto:info@photonsurgicalsystems.co.uk)

web: [www.photonsurgicalsystems.co.uk](http://www.photonsurgicalsystems.co.uk)